



**BIOELECTRICAL
SIGNAL
PROCESSING IN
CARDIAC AND
NEUROLOGICAL
APPLICATIONS**

**Leif Sörnmo
Pablo Laguna**

**BIOELECTRICAL SIGNAL PROCESSING
IN CARDIAC AND NEUROLOGICAL
APPLICATIONS**

This Page Intentionally Left Blank

BIOELECTRICAL SIGNAL PROCESSING IN CARDIAC AND NEUROLOGICAL APPLICATIONS

Leif Sörnmo

Department of Electrical Engineering

Lund University

Lund, Sweden

Pablo Laguna

Department of Electrical Engineering and

Aragón Institute of Engineering Research

Zaragoza University

Zaragoza, Spain



ELSEVIER
ACADEMIC
PRESS

Amsterdam Boston Heidelberg London New York Oxford
Paris San Diego San Francisco Singapore Sydney Tokyo

Elsevier Academic Press
30 Corporate Drive, Suite 400, Burlington, MA 01803, USA
525 B Street, Suite 1900, San Diego, California 92101-4495, USA
84 Theobald's Road, London WC1X 8RR, UK

This book is printed on acid-free paper.

Cover designer: Neringa Stjernman

Copyright ©2005, Elsevier Inc. All rights reserved.

No part of this publication may be reproduced or transmitted in any form or by any means, electronic or mechanical, including photocopy, recording, or any information storage and retrieval system, without permission in writing from the publisher.

Permissions may be sought directly from Elsevier's Science & Technology Rights Department in Oxford, UK: phone: (+44) 1865 843830, fax: (+44) 1865 853333, e-mail: permissions@elsevier.co.uk. You may also complete your request on-line via the Elsevier homepage (<http://elsevier.com>), by selecting "Customer Support" and then "Obtaining Permissions."

Library of Congress Cataloging-in-Publication Data

Application submitted

British Library Cataloguing in Publication Data

A catalogue record for this book is available from the British Library

ISBN: 0-12-437552-9

For all information on all Elsevier Academic Press publications
visit our Web site at www.books.elsevier.com

Printed in the United States of America

05 06 07 08 09 10 9 8 7 6 5 4 3 2 1

Contents

Preface	vii
Chapter 1. Introduction	1
1.1 Biomedical Signal Processing: Objectives and Contexts . . .	2
1.1.1 Objectives	2
1.1.2 Contexts	4
1.2 Basics of Bioelectrical Signals	6
1.2.1 On the Cellular Level	6
1.2.2 On the Body Surface	9
1.2.3 Bioelectrical Signals	11
1.3 Signal Acquisition and Analysis	14
1.4 Performance Evaluation	16
1.4.1 Databases	17
1.4.2 Simulation	21
Bibliography	22
Chapter 2. The Electroencephalogram—A Brief Background	25
2.1 The Nervous System	27
2.1.1 Neurons	28
2.1.2 The Cerebral Cortex	30
2.2 The EEG—Electrical Activity Measured on the Scalp	31
2.2.1 EEG Rhythms and Waveforms	33
2.2.2 Categorization of EEG Activity	36
2.3 Recording Techniques	37
2.4 EEG Applications	39
2.4.1 Epilepsy	40
2.4.2 Sleep Disorders	44
2.4.3 Brain–Computer Interface	47
Bibliography	50

Chapter 3. EEG Signal Processing	55
3.1 Modeling the EEG Signal	55
3.1.1 Deterministic and Stochastic Signal Properties	55
3.1.2 Stochastic Properties	56
3.1.3 Linear, Stochastic Models	63
3.1.4 Nonlinear Modeling of the EEG	67
3.2 Artifacts in the EEG	71
3.2.1 Artifact Characteristics	73
3.2.2 Artifact Processing	76
3.2.3 Artifact Reduction Using Linear Filtering	77
3.2.4 Artifact Cancellation Using Linearly Combined Reference Signals	78
3.2.5 Adaptive Artifact Cancellation Using Linearly Combined Reference Signals	83
3.2.6 Artifact Cancellation Using Filtered Reference Signals	87
3.3 Nonparametric Spectral Analysis	91
3.3.1 Fourier-based Power Spectrum Analysis	92
3.3.2 Spectral Parameters	97
3.4 Model-based Spectral Analysis	103
3.4.1 The Autocorrelation/Covariance Methods	106
3.4.2 The Modified Covariance Method	110
3.4.3 Burg's Method	112
3.4.4 Performance and Design Parameters	116
3.4.5 Spectral Parameters	119
3.5 EEG Segmentation	125
3.5.1 Spectral Error Measure—The Periodogram Approach	128
3.5.2 Spectral Error Measure—The Whitening Approach . .	131
3.5.3 Segmentation Performance and Beyond	134
3.6 Joint Time–Frequency Analysis	135
3.6.1 The Short-Time Fourier Transform	137
3.6.2 The Ambiguity Function	142
3.6.3 The Wigner–Ville Distribution	147
3.6.4 General Time–Frequency Distributions—Cohen's Class	153
3.6.5 Model-based Analysis of Slowly Varying Signals	158
Bibliography	162
Problems	175
 Chapter 4. Evoked Potentials	 181
4.1 Evoked Potential Modalities	183
4.1.1 Auditory Evoked Potentials	185
4.1.2 Somatosensory Evoked Potentials	187
4.1.3 Visual Evoked Potentials	188

4.1.4	Evoked Potentials and Cognition	189
4.2	Noise Characteristics	190
4.3	Noise Reduction by Ensemble Averaging	192
4.3.1	Averaging of Homogeneous Ensembles	193
4.3.2	Ensemble Averaging Interpreted as Linear Filtering	200
4.3.3	Exponential Averaging	202
4.3.4	Averaging of Inhomogeneous Ensembles	207
4.3.5	Spike Artifacts and Robust Averaging	219
4.3.6	The Effect of Latency Shifts	225
4.3.7	Estimation of Latency Shifts	229
4.3.8	Weighting of Averaged Evoked Potentials Using Ensemble Correlation	236
4.4	Noise Reduction by Linear Filtering	241
4.4.1	Time-Invariant, A Posteriori Filtering	243
4.4.2	Limitations with Time-Invariant, A Posteriori Filtering	252
4.5	Single-Trial Analysis Using Basis Functions	253
4.5.1	Orthogonal Expansions	254
4.5.2	Sets of Basis Functions	260
4.5.3	Karhunen–Loève Expansion—Optimal Basis Functions	264
4.5.4	Interpretation as Linear, Time-Variant Filtering	271
4.5.5	Modeling with Damped Sinusoids	272
4.6	Adaptive Analysis Using Basis Functions	278
4.6.1	The Instantaneous LMS Algorithm	279
4.6.2	The Block LMS Algorithm	285
4.7	Wavelets	286
4.7.1	The Wavelet Transform	288
4.7.2	Multiresolution Signal Analysis	292
4.7.3	Multiresolution Signal Analysis—A Classical Example	297
4.7.4	Implementation of the Discrete Wavelet Transform Using Filter Banks	300
4.7.5	Wavelet Examples	306
4.7.6	Denoising	312
	Bibliography	318
	Problems	329
Chapter 5.	The Electromyogram	337
5.1	The Electrical Activity of Muscles	338
5.1.1	Action Potentials and Motor Units	338
5.1.2	Recording of Myoelectric Signals	343
5.1.3	EMG Applications	345
5.2	Amplitude Estimation in the Surface EMG	347

5.2.1	Signal Model and ML Estimation	347
5.2.2	Modifications of the ML Amplitude Estimator	352
5.2.3	Multiple Electrode Sites	356
5.3	Spectral Analysis of the Surface EMG	361
5.4	Conduction Velocity Estimation	365
5.4.1	Two-Channel Time Delay Estimation	367
5.4.2	Multichannel Time Delay Estimation	369
5.5	Modeling the Intramuscular EMG	371
5.5.1	A Signal Model of the MUAP Train	372
5.5.2	MUAP Train Amplitude	377
5.5.3	MUAP Train Power Spectrum	378
5.6	Intramuscular EMG Signal Decomposition	383
5.6.1	MUAP Feature Extraction and Clustering	387
5.6.2	Resolution of Superimposed MUAP Waveforms	391
	Bibliography	398
	Problems	406
Chapter 6.	The Electrocardiogram—A Brief Background	411
6.1	Electrical Activity of the Heart	412
6.2	Generation and Recording of an ECG	415
6.2.1	Depolarization and Repolarization	415
6.2.2	ECG Recording Techniques	419
6.2.3	ECG Waves and Time Intervals	426
6.3	Heart Rhythms	430
6.3.1	Sinus Rhythm	431
6.3.2	Premature Beats	433
6.3.3	Atrial Arrhythmias	434
6.3.4	Ventricular Arrhythmias	436
6.3.5	Conduction Blocks	438
6.4	Heartbeat Morphologies	438
6.4.1	Myocardial Ischemia	438
6.4.2	Myocardial Infarction	439
6.5	Noise and Artifacts	440
6.6	Clinical Applications	443
6.6.1	Resting ECG	443
6.6.2	Intensive Care Monitoring	444
6.6.3	Ambulatory Monitoring	444
6.6.4	Stress Test	445
6.6.5	High-Resolution ECG	447
	Bibliography	449

Chapter 7. ECG Signal Processing	453
7.1 Baseline Wander	457
7.1.1 Linear, Time-Invariant Filtering	458
7.1.2 Linear, Time-Variant Filtering	467
7.1.3 Polynomial Fitting	470
7.2 Powerline Interference (50/60 Hz)	473
7.2.1 Linear Filtering	473
7.2.2 Nonlinear Filtering	476
7.2.3 Estimation-Subtraction	479
7.3 Muscle Noise Filtering	484
7.4 QRS Detection	485
7.4.1 Signal and Noise Problems	487
7.4.2 QRS Detection as an Estimation Problem	488
7.4.3 Detector Preprocessing	497
7.4.4 Decision Rules	504
7.4.5 Performance Evaluation	507
7.5 Wave Delineation	510
7.6 Data Compression	514
7.6.1 Lossless Compression	517
7.6.2 Lossy Compression—Direct Methods	519
7.6.3 Lossy Compression—Transform-based Methods	526
7.6.4 Interbeat Redundancy	533
7.6.5 Interlead Redundancy	536
7.6.6 Quantization and Coding	539
7.6.7 Performance Evaluation	541
Bibliography	545
Problems	557
 Chapter 8. ECG Signal Processing: Heart Rate Variability	 567
8.1 Acquisition and RR Interval Conditioning	568
8.2 Time Domain Measures	570
8.3 Heart Rhythm Representations	573
8.3.1 The Integral Pulse Frequency Modulation Model	574
8.3.2 Interval Series Representations	578
8.3.3 Event Series Representation	582
8.3.4 Heart Timing Representation	585
8.4 Spectral Analysis of Heart Rate Variability	589
8.4.1 Direct Estimation from Unevenly Spaced Samples	592
8.4.2 The Spectrum of Counts	593
8.4.3 Lomb's Periodogram	597
8.5 Clustering of Beat Morphologies	603
8.6 Dealing with Ectopic Beats	605

8.6.1	Correlation-based Correction	608
8.6.2	Interpolation-based Correction	609
8.6.3	The Heart Timing Signal and Ectopic Beats	611
8.7	Interaction with Other Physiological Signals	614
	Bibliography	621
	Problems	628
Appendix A. Review of Important Concepts		633
A.1	Matrix Fundamentals	633
A.1.1	Definitions	633
A.1.2	Matrix Decomposition	638
A.1.3	Matrix Optimization	640
A.1.4	Linear Equations	641
A.2	Discrete-Time Stochastic Processes	642
A.2.1	Definitions	642
A.2.2	Stationarity	644
A.2.3	Ergodicity	645
A.2.4	Bias and Consistency	645
A.2.5	Power Spectrum	646
A.2.6	White Noise	646
A.2.7	Filtering of Stochastic Processes	647
	Bibliography	648
Appendix B. Symbols and Abbreviations		649
B.1	Mathematical Symbols	649
B.2	Abbreviations	658
Index		661

Preface

Bioelectrical signals have been recorded and analyzed for several decades but still continue to excite physicians and engineers. Novel signal processing techniques have helped uncover information which completely changed the way various diseases previously were diagnosed. In fact, it is today difficult to imagine a situation when diseases related to the heart, the brain, or the muscles are diagnosed without also including certain information derived from bioelectrical signals. Such information is essential to therapeutic devices in cardiac, neurological, and neuromuscular applications, and will in the future, when systematically fused with other types of biomedical signals, continue to improve the quality of life of many patients. Monitoring of home-based patients is becoming increasingly popular in health care, frequently involving bioelectrical signals which can be safely and comfortably recorded using noninvasive techniques.

The aim of this book is to present a comprehensive overview of techniques with particular relevance to the processing of bioelectrical signals. The presentation is problem-driven and deals with issues having received considerable attention from both a scientific viewpoint, i.e., in the form of publications and conference presentations, and a viewpoint of product development. Since biomedical signal processing has been largely synonymous with the processing of ECG, EEG, EMG, and evoked potentials, we have focused the presentation on issues related to these four types of bioelectrical signals. It is yet our conviction that the reader is fully capable of transferring the way of thinking developed herein for bioelectrical signals, as well as to transfer the developed methods, when later dealing with other types of biomedical signals.

Choosing a problem-driven presentation means, in this book, that different methods are described within the context of a certain bioelectrical signal. For example, power spectral analysis is described within the context of EEG signal processing though such analysis is certainly well-established in other biomedical applications as well. While some may feel that the realm of a method's usefulness is depreciated with this kind of presentation, we hope nonetheless that the power in connecting a particular type of signal to a

particular method outweighs the disadvantages. On occasion, the problem-driven presentation also means the display of a smorgasbord of methods developed to solve a certain problem such as the cancellation of powerline interference. We hope that this way of dealing with a problem would serve the reader well by offering an idea of the diversity with which a problem can be solved. Not all methods considered in this textbook are directly applicable in clinical practice but may require one or several heuristic add-ons before their performance become satisfactory; the exact definition of such add-ons is rarely disclosed in the original publication of a method but needs to be developed by those interested in the method's pursuit.

With the display of different methods for solving a particular problem comes the natural wish of knowing which method offers the best performance. We have, however, abstained from making such comparisons due to the many pitfalls associated with choosing performance measure, data set, and so forth. We would instead like to challenge the reader to delve into this important aspect.

Biomedical signal processing has today reached certain maturity as an academic subject and is now supported by the availability of a handful of textbooks. Being an interdisciplinary subject by nature, biomedical signal processing has to be taught quite differently depending on the educational program. For students in biomedical engineering a course in physiology is part of the curriculum, whereas students in electrical engineering and computer science usually lack such a course. In order to maintain the interdisciplinary nature when teaching the latter group of students, we have included chapters or sections with brief, self-contained introductions to the underlying electrophysiology, recording techniques, and some important clinical applications. Without any prior knowledge of these aspects, a course in biomedical signal processing runs the risk of losing its very essence.

It is evident that a course on biomedical signal processing may embrace widely different contents—an observation which not only applies to the choice of biomedical signals but also to the choice of methodologies. Rather than yield to the temptation to include as much as possible, we have deliberately avoided to cover certain important techniques including pattern recognition, artificial neural networks, higher-order statistics, and nonlinear dynamics. Though important in biomedical applications, the fundamentals of these techniques are well-covered by a number of textbooks.

This book is intended for final year undergraduate students and graduate students in biomedical engineering, electrical engineering, and computer science. It is suitable for a one-quarter or one-semester course depending on the content covered and the amount of emphasis put on problem solving and project work. A necessary prerequisite is the fundamentals of digital signal processing as presented in textbooks such as [1, 2]. Since many re-

cent methods used in biomedical applications are based on concepts from statistical modeling and signal processing, a basic course in probability theory and stochastic processes is another important prerequisite. It is also desirable that the reader has certain familiarity with linear algebra so that common matrix operations (summarized in Appendix A) can be performed. Readers who want to achieve a deeper understanding of statistical signal processing are referred to a number of highly recommended textbooks on this topic [3–5]. Adaptive filtering is a topic which is just briefly touched upon in this book; comprehensive coverage of such filters and their properties can be found in [6].

This book may also be used as a comprehensive reference for practicing engineers, physicians, researchers and, of course, anyone interested in finding out what information can be derived from bioelectrical signals. For practicing engineers, we have used selected parts of the book for a short course on biomedical signal processing (i.e., 2–3 days); in such cases, the main emphasis should be put on the significance of different methods rather than on mathematical details.

Contents Overview

Chapter 1 puts biomedical signal processing in context, and gives a brief description of bioelectricity and its manifestation on the body surface as signals. General aspects on signal acquisition and performance evaluation are briefly considered.

Chapter 2 provides the reader with the basics of the brain, serving as a background to the following chapter on EEG signal processing. Some common EEG patterns are described and their relationships to cerebral pathology are pointed out. An understanding of EEG signal characteristics, as well as the purposes for which the characteristics can be exploited, is essential information when assimilating the contents of Chapter 3. The main themes in Chapter 3 on EEG signal processing are related to artifact rejection and spectral analysis; two techniques of critical importance to EEG interpretation. Special attention is given to the multitude of spectral analysis techniques and a section on time–frequency analysis is included.

Chapter 4 provides a comprehensive overview of noise reduction techniques for use with event-related signals, here treated within the context of evoked potentials. Similar to EEG signals and spectral analysis, evoked potentials and signal averaging became “partners” at a very early stage in the history of biomedical signal processing, thus motivating the emphasis on this partnership. The overview of noise reduction techniques covers both ensemble averaging (and its spawn) and more advanced approaches where

the signal is modeled and filtered using a basis function expansion; wavelets represent one such popular approach.

Chapter 5 deals with myoelectric activity and the related EMG signal recorded either by noninvasive or invasive techniques (and makes a minor departure from the general framework of dealing with signals recorded on the body surface). Of the many developed methods for EMG signal analysis, we cover some central ones related to muscle force and conduction velocity where signal modeling and statistical estimation techniques are involved.

Chapter 6 contains a background to the electrophysiology of the heart, describes the main characteristics of the ECG signal in terms of morphology and rhythm, and prepares the way for Chapters 7 and 8 by mentioning the most important ECG applications. Chapter 7 describes a suite of methods, essential to any system which performs ECG signal analysis, developed for the purpose of noise reduction, heartbeat detection and delineation, and data compression. Chapter 8 is completely devoted to the analysis of heart rate variability—an area of considerable clinical and technical interest in recent years—and describes techniques for representing and characterizing such variability in the time and frequency domain.

We have included an extensive, but not exhaustive, number of references which give the interested reader rich possibilities to further explore the original presentations of the methods. References are almost exclusively made to journal publications since these are easily retrieved from libraries. As a result, the very first publication of a method, often appearing in a conference proceeding, is not acknowledged for which we apologize.

A collection of problems has been developed in order to illustrate the presented methods and their applications. While some problems are straightforward to solve, others require considerable effort and background knowledge and are intended as “appetizers” for students interested in pursuing research in biomedical signal processing. An accompanying manual with detailed solutions to all problems is available at the publisher’s web site

www.books.elsevier.com/0124375529

to instructors who adopt the book.

Any course on biomedical signal processing must include one or several projects which give the student an opportunity to process signals and to learn the pros and cons of a method. We have developed a companion web site where several project descriptions are listed and signals available for download; its location is

www.biosignal.lth.se

An important goal with this web site is to allow the inclusion of new projects so that projects can be submitted by anyone interested in teaching the contents of this book (submission instructions are available at the web site).

Those interested in using this book for a one-quarter course may want to omit the sections on time–frequency analysis (Section 3.6), basis functions and related adaptive analysis (Sections 4.5 and 4.6), wavelets (Section 4.7), and certain parts of Chapter 8 dealing with heart rate variability; the mathematical level is relatively advanced in all these parts. A shorter course may to a lesser extent deal with problem solving, however, we strongly encourage the inclusion of at least one project since it provides the student with experiences essential to the understanding of biomedical signal processing.

Acknowledgments

The making of an interdisciplinary textbook is only possible with the help of many people. We are fortunate to have colleagues and friends who, most generously, have supported us with their expertise and helpful advices.

We would like to express our deep gratitude to Juan Pablo Martínez (Zaragoza), Olivier Meste (Nice), Salvador Olmos (Zaragoza), and Olle Pahlm (Lund), who willingly reviewed the material in different parts of the manuscript and provided us with numerous suggestions and corrections. Their profound understanding of biomedical signals has considerably contributed to improve the manuscript.

We are grateful for the input given by Jan Anders Ahnslide (Lund), Magnus Lindgren (Oslo), Miguel Angel Mañanas (Barcelona), and Roberto Merletti (Torino); their expertise in the areas of neurophysiology and electromyography has been invaluable when preparing the parts of the book concerning these aspects. We are also grateful to Vaidotas Marozas (Kaunas), Nitish Thakor (Baltimore), and Patrik Wahlberg (Lund); they read parts of the manuscript and provided us with helpful comments and unique perspectives on biomedical signal processing.

We would like to acknowledge the helpful comments and feedback from our doctoral students; special thanks goes to Joakim Axmon, Javier Mateo, Frida Nilsson, Kristian Solem, Martin Stridh, and Magnus Åström, for proof-reading, designing problems and projects, and providing us with data. Since this course was introduced some five years ago at our universities, we have received several comments from our students to whom we would like to express our appreciation; in particular, we thank Åsa Robertsson for help with Matlab programming.

We also wish to thank Rute Almeida (Porto), Ed Berbari (Indianapolis), Per Ola Börjesson (Lund), Christina Grossmann (Lund), Bo Hjorth (Stock-

holm), Arturas Janušauskas (Kaunas), Algimantas Krisčiukaitis (Kaunas), Gerhard Kristensson (Lund), Arunas Lukosevičius (Kaunas), Jonas Pettersson (Lund), Ana Paula Rocha (Porto), Helen Sheppard (Lund), Owe Svensson (Lund), and Viktor Öwall (Lund). Their different talents contributed significantly to improve the content of this book.

We are grateful to Kerstin Brauer (Lund) for skillfully helping us with the illustrative figures, and to Lena Eliasson (Lund) for preparing Figure 1.1. A number of figures are based on signals which generously were made available to us; Stefan Sauermann (Vienna) provided the signals for Figure 1.4(a) and (c), Jan Anders Ahnslide (Lund) for Figure 1.4(b), and José Luis Martínez de Juan (Valencia) for Figure 1.5(b). We are also grateful to Fabrice Wendling (Rennes) who made Figure 3.6 available, Nils Löfgren (Borås) for Figure 3.31, Patrick Celka (Neuchâtel) for Figure 3.38, Rodrigo Quian Quiroga (Leicester) for Figure 4.49, Maria Hansson (Lund) for Figure 6.13, Franc Jager (Ljubljana) for Figure 8.1, and Luca Mainardi (Milano) for Figure 8.24.

Special thanks are due to Christine Minihane and the staff at Elsevier for their cooperation and continuing encouragement during the authoring and production process.

The Spanish government kindly provided financial support through the grants SAB2003-0130 and TXT1996-1793. Support was also received from the European Community through the SOCRATES/ERASMUS Teaching Staff Mobility program.

We are infinitely grateful to our respective families for their support and encouragement throughout this project. Above all, we admire their endless patience when we got lost in yet another discussion on “the book.” Parts of the manuscript were conceived in a picturesque village of the Spanish Pyrenees; we would like to express our sincere thanks to relatives and friends living there who made these occasions productive and highly enjoyable.

We are deeply indebted to artist Neringa Stjernman who enriched the book cover by her interpretation of bioelectrical signals; it was a great surprise, and a pure joy, to find out about her unique relationship to electrophysiology. It would be incomplete not to acknowledge the influence of Palle Mikkelborg whose music has been a vital source of inspiration in the making of this book. His trumpet paints a spectrum full of colors—blue in green, orange with electric red, anything but grey—which makes one sing a song.

Leif Sörnmo
Pablo Laguna

Bibliography

- [1] J. G. Proakis and D. G. Manolakis, *Digital Signal Processing. Principles, Algorithms, and Applications*. New Jersey: Prentice-Hall, 3rd ed., 1996.
- [2] A. V. Oppenheim, R. W. Schaffer, and J. R. Buck, *Discrete-Time Signal Processing*. New Jersey: Prentice-Hall, 2nd ed., 1999.
- [3] C. W. Therrien, *Discrete Random Signals and Statistical Signal Processing*. New Jersey: Prentice-Hall, 1992.
- [4] S. M. Kay, *Fundamentals of Statistical Signal Processing. Estimation Theory*. New Jersey: Prentice-Hall, 1993.
- [5] M. Hayes, *Statistical Digital Signal Processing and Modeling*. New York: John Wiley & Sons, 1996.
- [6] S. Haykin, *Adaptive Filter Theory*. New Jersey: Prentice-Hall, 4th ed., 2002.

This Page Intentionally Left Blank

Chapter 1

Introduction

The function of the human body is frequently associated with signals of electrical, chemical, or acoustic origin. Such signals convey information which may not be immediately perceived but which is hidden in the signal's structure. This information has to be “decoded” or extracted in some way before the signals can be given meaningful interpretations. The signals reflect properties of their associated underlying biological systems, and their decoding has been found very helpful in explaining and identifying various pathological conditions. The decoding process is sometimes straightforward and may only involve very limited, manual effort such as visual inspection of the signal on a paper print-out or computer screen. However, the complexity of a signal is often quite considerable, and, therefore, biomedical signal processing has become an indispensable tool for extracting clinically significant information hidden in the signal.

Biomedical signal processing represents an interdisciplinary topic. Knowledge of the physiology of the human body is crucial to avoid the risk of designing an analysis method which distorts, or even removes, significant information. It is also valuable to have a sound knowledge of other topics such as anatomy, linear algebra, calculus, statistics, and circuit design.

Biomedical signal processing has, by some, been viewed as a stepping-stone for developing diagnostic systems which offer fully automated analysis. Some decades ago when computers first arrived in the area of medicine, automation was the overriding goal. However, this goal has been considerably modified over the years, not only because of the inherent difficulties in developing such systems, but equally so because the physician must be ultimately responsible for the diagnostic decisions taken. While fully automated analysis may be warranted in a few situations, today's goal is rather to develop computer systems which offer advanced aid to the physician in making well-

founded decisions. In these systems biomedical signal processing has come to play a very important role.

Research in biomedical signal processing has so far mainly been concerned with the analysis of one particular signal type at a time (“unimodal signal analysis”); a fact, which to a large extent, influences the content of the present textbook. However, the emerging interest in multimodal signal analysis will definitely help to explain, in more detail, how different physiological subsystems interact with each other, such as the interaction between blood pressure and heart rate in the cardiovascular system. By exploring the mutual information contained in different signals, more qualified diagnostic decisions can be made. The increased algorithmic complexity associated with multimodal analysis is not a serious limitation since it will be met by the rapid advancement of computer technology and the ever-increasing computational speed.

1.1 Biomedical Signal Processing: Objectives and Contexts

1.1.1 Objectives

Biomedical signal processing has many objectives, and some of the most important ones are presented below. We also describe the main contexts in which biomedical signal processing is applied. Other challenging objectives and contexts can certainly be defined by those interested in pursuing a career in this fascinating, interdisciplinary field.

Historically, biomedical signals have often been assessed visually, and manual ruler-based procedures were developed to make sure that measurements could be obtained in a standardized manner. However, it is well-known that there is relatively poor concordance between manually obtained measurements, and this may lead to unreliable diagnostic conclusions. A fundamental objective of biomedical signal processing is therefore to *reduce the subjectivity* of manual measurements. The introduction of computer-based methods for the purpose of objectively quantifying different signal characteristics is the result of a desire to improve measurement accuracy as well as reproducibility.

In addition to reducing measurement subjectivity, biomedical signal processing is used in its own right for developing methods that *extract features* to help characterize and understand the information contained in a signal. Such feature extraction methods can be designed to mimic manual measurements, but are equally often designed to extract information which is not readily available from the signal through visual assessment. For example,

small variations in heart rate that cannot be perceived by the human eye have been found to contain very valuable clinical information when quantified in detail using a suitable signal processing technique; see Chapter 8 for more details on this particular topic. Although it is certainly desirable to extract features that have an intuitive meaning to the physician, it is not necessarily those features which yield the best performance in clinical terms.

In many situations, the recorded signal is corrupted by different types of noise and interference, sometimes originating from another physiological process of the body. For example, situations may arise when ocular activity interferes with the desired brain signal, when electrodes are poorly attached to the body surface, or when an external source such as the sinusoidal 50/60 Hz powerline interferes with the signal. Hence, *noise reduction* represents a crucial objective of biomedical signal processing so as to mitigate the technical deficiencies of a recording, as well as to separate the desired physiological process from interfering processes. In fact, the desired signal is in certain situations so dramatically masked by noise that its very presence can only be revealed once appropriate signal processing has been applied. This is particularly evident for certain types of transient, very low-amplitude activity such as evoked potentials, which are part of brain signals, and late potentials, which are part of heart signals.

Certain diagnostic procedures require that a signal be recorded on a long timescale, sometimes lasting for several days. Such recordings are, for example, routinely done for the purpose of analyzing abnormal sleep patterns or to identify intermittently occurring disturbances in the heart rhythm. The resulting recording, which often involves many channels, amounts to huge data sizes, which quickly fill up hard disk storage space once a number of patients have been examined. Transmission of biomedical signals across public telephone networks is another, increasingly important application in which large amounts of data are involved. For both these situations, *data compression* of the digitized signal is essential and, consequently, another objective of biomedical signal processing. General-purpose methods of data compression, such as those used for sending documents over the internet, do not perform particularly well since the inherent characteristics of the biomedical signal are not at all exploited. Better performance can be obtained by applying tailored algorithms for data compression of biomedical signals. Data compression can also be understood in a wider sense as the process in which clinical information from a long-term recording is condensed into a smaller data set that is more manageable for the person analyzing the data. In this latter sense, it is highly desirable to develop signal processing algorithms which are able to determine and delimit clinically significant episodes.

Mathematical *signal modeling* and *simulation* constitute other important objectives in biomedical signal processing which can help to attain a bet-

ter understanding of physiological processes. With suitably defined model equations it is possible to simulate signals which resemble those recorded on the cellular level or on the body surface, thereby offering insight into the relationship between the model parameters and the characteristics of the observed signal. Examples of bioelectrical models include models of the head and brain for localizing sources of neural activity and models of the thorax and the heart for simulating different cardiac rhythms. Signal modeling is also central to the branch of signal processing called “model-based signal processing,” where algorithm development is based on the optimization of an appropriately selected performance criterion. In employing the model-based approach, the suggested signal model is fitted to the observed signal by selecting those values of the model parameters which optimize the performance criterion. While model-based biomedical signal processing represents a systematic approach to the design of algorithms—to be frequently adopted in the present textbook—it does not always lead to superior performance; heuristic approaches may actually perform just as well and sometimes even better. It is a well-known fact that many commercial, medical devices rely on the implementation of ad hoc techniques in order to achieve satisfactory performance.

The complexity of a signal model depends on the problem to be solved. In most signal processing contexts, it is fortunately not necessary to develop a multilevel model which accounts for cellular mechanisms, current propagation in tissue, and other biological properties. Rather, it is often sufficient to develop a “phenomenological” model which only accounts for phenomena which are relevant to the specific problem at hand.

1.1.2 Contexts

The other purpose of this section is to point out the three major clinical contexts in which algorithms for biomedical signal processing are designed, namely, the contexts of

- *diagnosis*,
- *therapy*, and
- *monitoring*.

In the *diagnostic context*, medical conditions are identified from the examination of signal information, reflecting the function of an organ such as the brain or the heart, in combination with other symptoms and clinical signs. A signal is often acquired by a noninvasive procedure which makes the examination less taxing on the patient. Most of these procedures are also associated with inexpensive technology for acquisition and analysis, thus

increasing the likelihood that the technology can be disseminated to countries with less developed economies. A diagnostic decision rarely requires immediate availability of the results from signal analysis, but it is usually acceptable to wait a few minutes for the analysis to be completed. Hence, signal analysis can be done off-line on a personal computer, thus relying on standardized hardware and operating system, possibly supplemented with a digital signal processor (DSP) board for accelerating certain bottleneck computations. Algorithms for biomedical signal processing do not define the entire diagnostic computer system, but their scope ranges from performing a simple filtering operation to forming a more substantial part of the clinical decision-making.

Therapy generally signifies the treatment of disease and often involves drug therapy or surgery. With regard to biomedical signal processing, therapy may imply a narrower outlook in the sense that an algorithm is used to directly modify the behavior of a certain physiological process, for example, as the algorithms of a pacemaker do with respect to cardiac activity. In a therapeutic context, an algorithm is commonly designed for implementation in an implantable device like a heart defibrillator, and, therefore, it must, unlike an algorithm operating in a diagnostic context, strictly comply with the demands of on-line, real-time analysis. Such demands pose some serious constraints on algorithmic complexity as well as on the maximal acceptable time delay before a suitable action needs to be taken. Low power consumption is another critical factor to be considered in connection with devices that are implanted through a surgical procedure; for example, the battery of an implantable device is expected to last up to ten years. Hence, algorithms which involve computationally demanding signal processing techniques are less suitable for use in a therapeutic context.

Biomedical signal processing algorithms form an important part of real-time systems for *monitoring* of patients who suffer from a life-threatening condition. Such systems are usually designed to detect changes in cardiac or neurological function and to predict the outcome of a patient admitted to the intensive care unit (ICU). Since such changes may be reversible with early intervention, irreversible damage can sometimes be prevented. Similar to therapeutic contexts, the signal is processed during monitoring in an essentially sequential fashion such that past samples constitute the main basis for a decision, while just a few seconds of the future samples may also be considered—a property which usually stands in sharp contrast to signal processing for diagnostic purposes, where the signal is acquired in its entirety prior to analysis. Thus, a noncausal approach to signal analysis can only be adopted in the diagnostic context which mimics that of a human reader who interprets a signal by making use of both past and future properties. Constraints need to be imposed on the algorithmic design in terms of max-

imal delay time because the occurrence of a life-threatening event must be notified to the ICU staff within a few seconds. Another important issue to be considered is the implications of a clinical event that is missed by the algorithm or the implications of a nonevent that is falsely detected causing the staff to be notified.

1.2 Basics of Bioelectrical Signals

Although the scope of the present textbook is to present signal processing techniques useful for the analysis of electrical signals recorded on the *body surface*, it may still be well-motivated to consider the genesis of bioelectrical signals from a cellular perspective. Bioelectrical signals are related to ionic processes which arise as a result of electrochemical activity of a special group of cells having the property of *excitability*. The mechanisms which govern the activity of such cells are similar, regardless of whether the cells are part of the brain, the heart, or the muscles. In particular, the electrical force of attraction has central importance for the processing and transmission of information in the nervous system, as well as for sustaining the mechanical work done by the heart and the muscles. Since the origin of these voltages is only briefly described below, the interested reader is referred to textbooks on human physiology which offer a much more detailed description of the cellular aspects [1, 2]. The basic concepts introduced for mathematical modeling of bioelectrical phenomena are described in [3], while more comprehensive reading is found in [4–6].

1.2.1 On the Cellular Level

A cell is bounded by a plasma membrane which basically consists of lipid layers with poor ability to conduct an electrical current. The membrane possesses permeability properties which allow certain substances to pass from the inside of the cell to the outside through different channels, defined by body fluids, while other substances remain blocked. Intracellular and extracellular fluids mainly consist of water, which is electrically neutral; however, the fluids become electrically conductive since they contain several types of ions. The dominant ions in a nerve cell (neuron) are sodium (Na^+), potassium (K^+), and chloride (Cl^-). Other ions such as calcium (Ca^{2+}) are also present but play roles of varying importance depending on where the excitable cell is located; the calcium ion is much more important in the cells of the heart than in the nerves, for example.

Under resting conditions, the inside of a cell is negatively charged with respect to the outside, and, therefore, a negative transmembrane potential results since the outside is assumed to have zero voltage. The difference in

charge is due to the fact that the concentration of negatively charged ions inside the cell is higher than on the outside, whereas the opposite relation applies to the concentration of positive ions. In addition to the difference in ion concentration, the actual magnitude of the resting transmembrane potential is also determined by the permeability of the membrane to the different ions.

A potential arises when membrane channels open so that a certain ion may diffuse across the membrane. This process can be illustrated by the simplified situation in which potassium ions are assumed to be inside the cell and sodium ions outside and when the initial transmembrane potential is equal to zero. When the potassium channels are opened, an increase in positive electrical charge outside the cell is created as a result of the diffusion process; at the same time, the inside of the cell becomes increasingly negative and a potential arises across the membrane. This electrical potential constitutes the other force which causes ions to move across the membrane. As the outside of the cell becomes increasingly positive, the resulting potential will increasingly influence the outbound movement of potassium ions. The ion movement ceases when the concentration force balances the electrical force; an equilibrium potential is then said to have been reached. It should be noted that some other active transport mechanisms, not considered here, also come into play when a potential is created.

The resting transmembrane potential of a cell is determined by the equilibrium potentials of the different ions involved and is thus not equal to any of the equilibrium potentials of an individual type of ion. For the situation considered above with open potassium channels, the equilibrium potential for potassium in a nerve cell is found to be about -90 mV, while the equilibrium potential for sodium—assuming instead open sodium channels—is about $+60$ mV. The resting transmembrane potential is within the range of -60 to -100 mV, depending on the type of cell.

When a cell is stimulated by a current, rapid alterations in membrane ion permeability take place which give rise to a change in the membrane potential and generate a signal referred to as an *action potential*. The propagation of action potentials is the very mechanism which makes the heart contract and the nervous system communicate over short and long distances. The stimulus current must exceed a certain threshold level in order to elicit an action potential, otherwise the cell will remain at its resting potential. An excited cell exhibits nonlinear behavior: once a stimulus intensity exceeds the threshold level the resulting action potential is identical and independent of intensity—the *all-or-nothing principle*. An action potential consists mainly of two phases: *depolarization* during which the membrane potential changes toward zero so that the inside of the cell becomes less negative, and ultimately reverses to become positive, and *repolarization* during which the

potential returns to its resting level so that the inside again becomes more negative.

The membrane potential remains at its resting level until it is perturbed by some external stimulus, such as a current propagating from neighboring cells. Depolarization is then initiated, and the membrane permeability changes so that sodium channels are opened and the sodium ions can rush into the cell. At the same time, potassium ions try to exit since these are concentrated on the inside, but cannot, thereby causing the charge inside the cell to become increasingly positive, and eventually the membrane potential reverses polarity. Once the rush of sodium ions into the cell has stopped and the membrane potential approaches the sodium equilibrium potential, the peak amplitude of an action potential is reached. During repolarization, sodium channels close and potassium channels open so that the membrane potential can return to its resting, negative potential. The activity of a potassium channel is illustrated in Figure 1.1.

The duration of an action potential varies much more than its amplitude: the repolarization phase of a cardiac cell is much longer than the depolarization phase and lasts from 200 to 300 milliseconds, while for a neuron the two phases combined only last for about one millisecond with both phases having about the same duration. Figure 1.2 shows the action potentials for cells of the brain (motor neuron), the skeletal muscle, and the heart. From these waveforms, it can be observed that the cardiac action potential differs considerably from the others in its lack of an immediate repolarization phase. Instead, there is a plateau in the action potential because the membrane channels of the different ions open and close at different speeds.

Once an action potential has been elicited, the membrane cannot immediately respond to a new stimulus but remains in a “refractory” state for a certain period of time. The refractory period is related to changes that take place in sodium and potassium permeability of the membrane. Obviously, the refractory period imposes an upper limit on the frequency at which action potentials can be communicated through the nervous system or the heart can beat.

The propagation of an action potential exhibits special behavior since it travels a distance through the triggering of new action potentials rather than by traveling itself along the membrane. The current created by the initial membrane depolarization triggers an adjacent membrane so that a new action potential results, and so on. This process repeats itself until the membrane ends and delivers an action potential which is identical to the initial action potential. Due to the refractory period, the action potential travels away from membranes which recently have been excited and continues to do so until it reaches a point on the membrane where the voltage is insufficient for further stimulation.

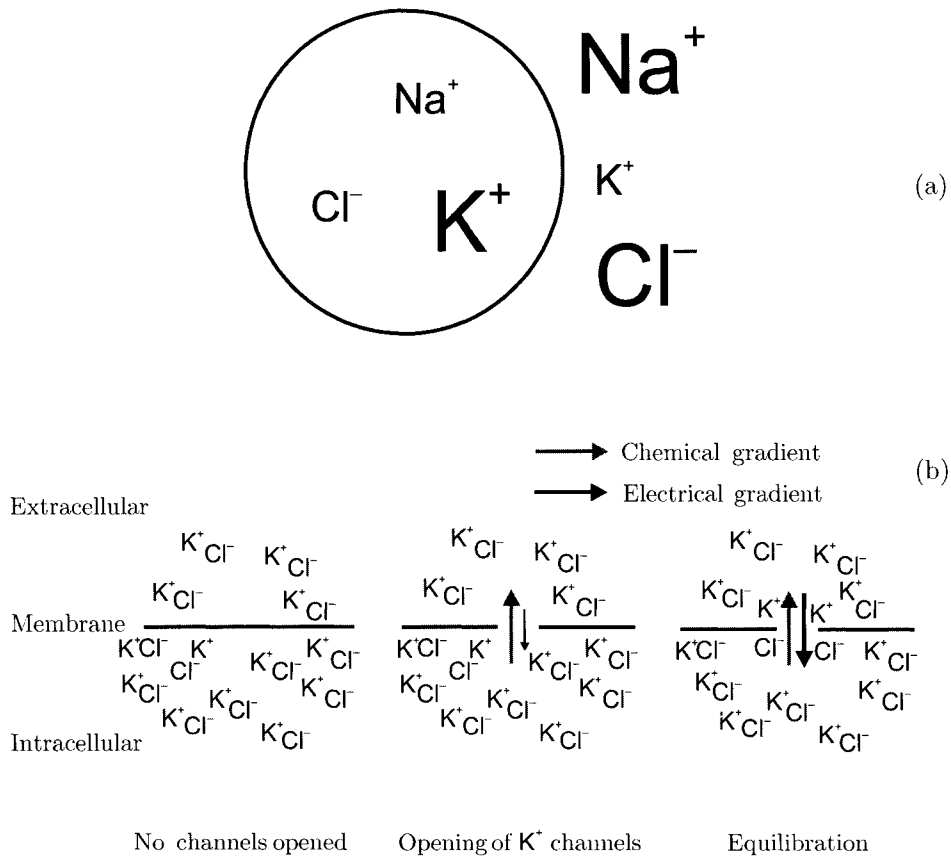


Figure 1.1: Cellular activity of potassium channels (which is similar for sodium but the reverse). (a) Concentration distribution of potassium (K^+), sodium (Na^+), and chloride (Cl^-) ions inside and outside a cell. (b) The relationship between chemical gradient and electrical gradient for K^+ ions and K^+ channels.

1.2.2 On the Body Surface

The ability of excitable cell membranes to generate action potentials causes a current to flow in the tissue that surrounds the cells. With the tissue being a conducting medium, commonly referred to as a volume conductor, the collective electrical activity of many cells can be measured noninvasively on the body surface [4–6]. The recording of a bioelectrical signal in clinical practice is done by attaching at least two electrodes to the body surface. In its simplest form, a signal is recorded by making use of two electrodes: the “exploring” electrode, placed close to the electrical source, and the “indifferent” electrode, placed elsewhere on the body surface [7]. Multiple electrode configurations are commonly used in clinical practice to obtain a spatial de-

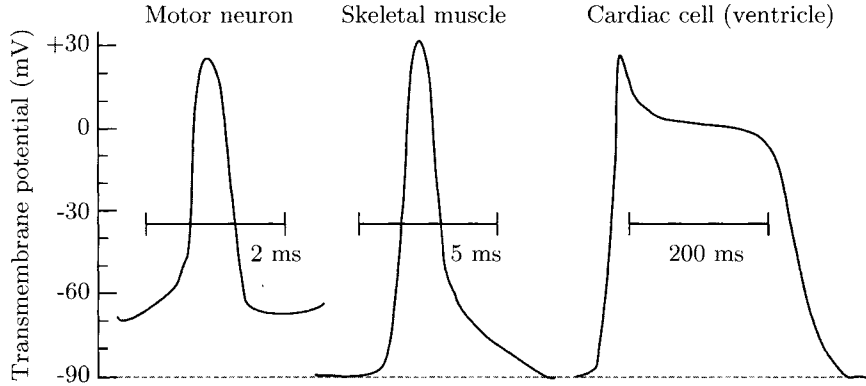


Figure 1.2: Examples of action potentials with shapes that range from the spike-like waveform of a nerve cell (left) to the much more extended waveform of a cardiac cell (right). The transmembrane potential difference was measured by placing one microelectrode inside the cell and another outside. It should be noted that the timescale differs from waveform to waveform.

scription of the bioelectrical phenomenon. Since the activity of excitable cells is viewed from a distance by the electrodes, with different tissues in between, such as blood, skeletal muscles, fat, and bone, it is impossible to noninvasively determine detailed information about cellular properties and propagation patterns. Nonetheless, significant empirical knowledge has over the years been acquired from analyzing the patterns of signals recorded on the body surface, which have been found crucial for clinical decision-making; this observation constitutes an important motivation for the writing of the present textbook.

The problem of characterizing the electrical source by noninvasive measurements has, in spite of the above-mentioned limitations, been the subject of considerable research due to the far-reaching clinical implications of its potential solution. In order to arrive at a meaningful solution, it is necessary to introduce a mathematical model in which the collective electrical cellular activity is treated as a volume source, i.e., it is defined by a fixed dipole, a multiple dipole, or some other source model. Furthermore, by introducing a model for the volume conductor which accounts for essential properties of the human body, such as geometry and resistivity, the electrical field measured on the body surface can be modeled. The important *inverse problem* consists of determining the electrical source from measurements on the body surface under the assumption that the geometry and electrical properties of the volume conductor are known [5].

1.2.3 Bioelectrical Signals

The present textbook deals with the processing of electrical signals that describe the activity of the brain, the heart, and the muscles. Some of these signals reflect spontaneous, ongoing activity, while others only occur as the result of external stimulation. The properties of these signals call for widely different processing techniques; an individual waveform can in some signals be directly linked to a specific clinical diagnosis, while in other signals the composite of many waveforms must be analyzed before a meaningful interpretation can be made.

The **electroencephalogram** (EEG) reflects the electrical activity of the brain as recorded by placing several electrodes on the scalp, see Figure 1.3(a). The EEG is widely used for diagnostic evaluation of various brain disorders such as determining the type and location of the activity observed during an epileptic seizure or for studying sleep disorders. The brain activity may also be recorded during surgery by attaching the electrodes directly to the uncovered brain surface; the resulting invasive recording is named an *electrocorticogram* (ECoG). The background to EEG signals is presented in Chapter 2 and is then followed by Chapter 3 where different EEG signal processing techniques are described.

Evoked potentials (EPs) constitute a form of brain activity which usually is evoked by a sensory stimulus such as one of visual or acoustic origin. Their clinical use includes the diagnosis of disorders related to the visual pathways and the brainstem. An EP, also referred to as an event-related potential, is a transient signal which consists of waves of such tiny amplitudes that its presence in the “background EEG” is typically invisible to the human eye, see Figure 1.4(a). Evoked potentials are recorded using an electrode configuration similar to that of an EEG. Chapter 4 contains an overview of methods developed for “revealing” EPs and for analyzing the resulting signal waveform.

The **electrocardiogram** (ECG) reflects the electrical activity of the heart and is obtained by placing electrodes on the chest, arms, and legs, see Figure 1.3(b). With every heartbeat, an impulse travels through the heart which determines its rhythm and rate and which causes the heart muscle to contract and pump blood. The ECG represents a standard clinical procedure for the investigation of heart diseases such as myocardial infarction. The *electrogram* (EG) is an intracardiac recording where the electrodes have been placed directly within the heart; the EG signal is used in implantable devices such as pacemakers and defibrillators. The background to ECG signals is presented in Chapter 6, while Chapters 7 and 8 present different ECG signal processing techniques.

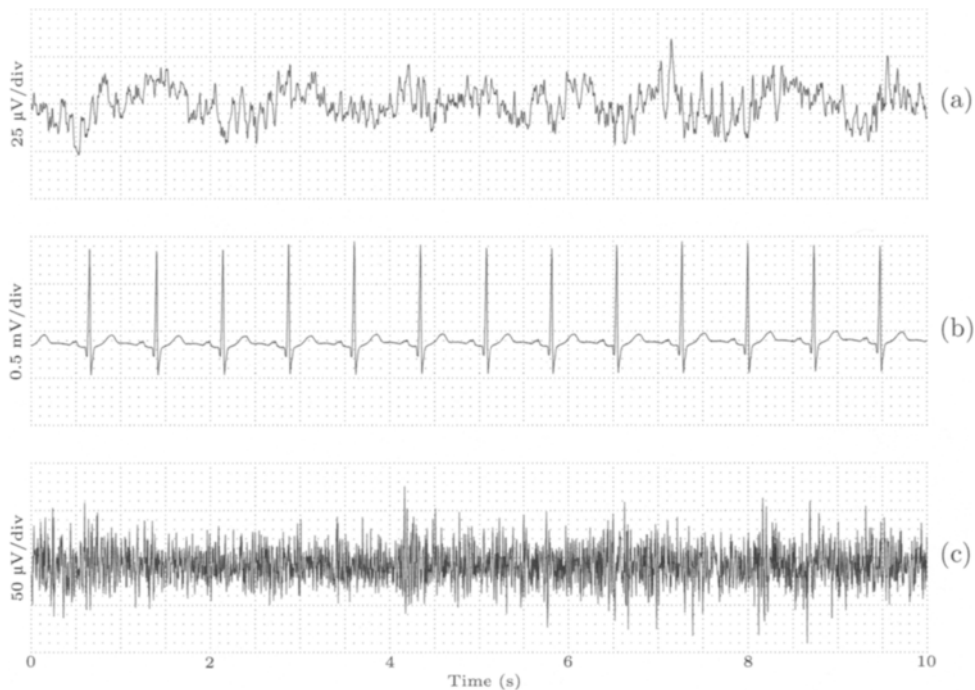


Figure 1.3: Examples of the three major bioelectrical signals recorded from the body surface: (a) an electroencephalogram (EEG) containing alpha activity, (b) an electrocardiogram (ECG) during sinus rhythm, and (c) an electromyogram (EMG) obtained from the chin in the waking state. All three signals were obtained from different normal subjects.

The **electromyogram** (EMG) records the electrical activity of skeletal muscles which produce an electrical current, usually proportional to the level of activity, see Figure 1.3(c). The EMG is used to detect abnormal muscular activity which occurs in many diseases such as muscular dystrophy, inflammation of muscles, and injury to nerves in arms and legs. Recording the surface EMG involves placing the electrodes on the skin overlying the muscle, whereas the intramuscular EMG involves inserting needle electrodes through the skin into the muscle to be examined. Chapter 5 presents an overview of EMG signal processing techniques.

Some other types of bioelectrical signals also deserve mentioning although their related signal analysis will not be further considered in the present textbook.

The *electroneurogram* (ENG) results from the stimulation of a peripheral nerve with an electric shock such that the response along the nerve can be measured. The ENG, usually acquired with needle electrodes, is used

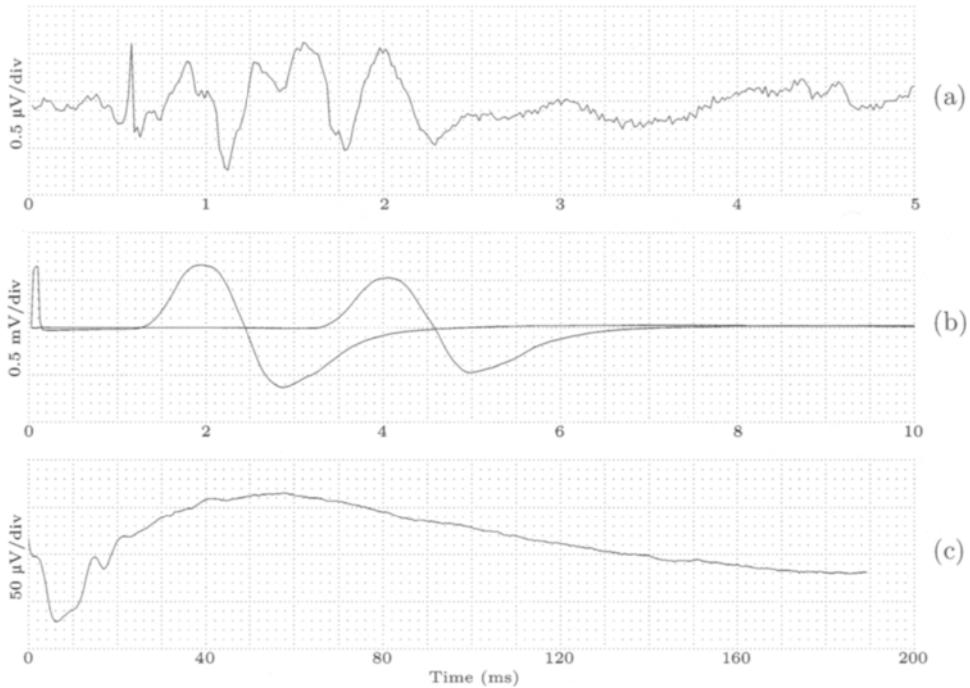


Figure 1.4: Examples of bioelectrical signals resulting from stimulation. (a) An evoked potential (EP) resulting from auditory stimulation (the brainstem response). The displayed signal is actually the result of averaging several responses in order to reduce the high noise level of the original signal; see Section 4.3 for details on noise reduction. (b) An electroneurogram (ENG) recorded at two electrode locations, where the delay between the two signals is used to estimate nerve conduction velocity. (c) An electroretinogram (ERG) obtained during stimulation with a flash of light.

to determine the conduction velocity of the nerve, thereby assisting in the diagnosis of nerve injury. By stimulating a nerve at two different sites separated by a well-defined distance, it is possible to estimate the conduction velocity from the distance by which the resulting two signal waveforms are separated, see the example in Figure 1.4(b). The ENG can be measured both invasively and noninvasively.

An *electroretinogram* (ERG) is used for studying the electrical potentials generated by the retina of the eye during light stimulation [8, 9], see Figure 1.4(c). The ERG is recorded by placing the exploring electrode, encapsulated in a contact lens, on the cornea. The ERG has been found useful for assessing the electrical response of the rods and cones, i.e., the visual cells at the back of the retina. A normal ERG shows appropriate responses

with increased light intensity, while an abnormal ERG is obtained in conditions such as arteriosclerosis of the retina or detachment of the retina. The algorithms described in Chapter 4 for signal processing of EPs are, by and large, also applicable to the analysis of ERGs.

The *electrooculogram* (EOG) is the recording of the steady corneal-retinal potential which is proportional to vertical and horizontal movements of the eye, thus offering an objective way to quantify the direction of the gaze [5, 10], see Figure 1.5(a). The EOG is of particular interest in patients who suffer from sleep disorders, where the presence of rapid eye movement (REM) is important for determining certain sleep stages. The EOG is recorded when studying nystagmus, i.e., a rapid, involuntary oscillation of the eyeballs, for example, in patients suffering from vertigo and dizziness. The EOG is also useful in virtual reality environments where a device for eye-tracking may be needed. The EOG is briefly touched upon in Chapter 3 in connection with EEG signal processing since the electrical activity caused by eye movements often interferes with the EEG and, therefore, needs to be cancelled.

The *electrogastrogram* (EGG) is a recording of the impulses which propagate through the muscles of the stomach and which control their contractions [11], see Figure 1.5(b). The EGG is studied when the muscles of the stomach or the nerves controlling the muscles are not working normally, for example, when the stomach does not empty food normally. The EGG is recorded by attaching a number of electrodes over the stomach during fasting and subsequent to a meal. In normal individuals a regular “rhythmic” signal is generated by the muscles of the stomach, having an amplitude which increases after a meal; the normal frequency of the gastric rhythm is approximately 3 cycles/minute. However, in symptomatic patients the rhythm is often irregular and sometimes without the increase in amplitude that follows a meal. A small selection of papers describing technical means of analyzing the EGG signal can be found in [12–16].

1.3 Signal Acquisition and Analysis

The acquisition of bioelectrical signals is today accomplished by means of relatively low-cost equipment which appropriately amplifies and digitizes the signal. As a result, several clinical procedures based on bioelectrical signals are in widespread use in hospitals around the world. In many situations, PC-based systems can be utilized as an efficient and cost-effective solution for signal analysis, especially considering the availability of expansion cards for data acquisition. Such a system includes one or several sensors, external hardware for patient insulation and signal amplification, an acquisition

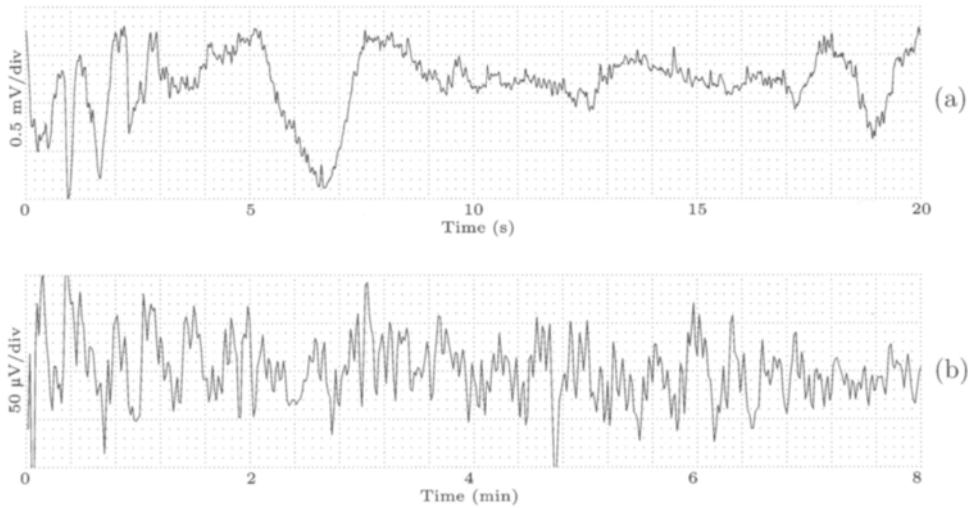


Figure 1.5: Recordings which exemplify (a) an electrooculogram (EOG) of the right eye and (b) an electrogastrogram (EGG). Note that the two timescales differ.

card with analog/digital (A/D) conversion, and software for signal analysis (Figure 1.6) [17]. In situations where the analysis is performed in an implantable device, the system design involves additional considerations, e.g., those related to the design of application-specific integrated circuitry and the selection of appropriate battery technology.

In the digitization process, it is usually sufficient to use 12–14 bits for amplitude quantization in order to cover the dynamic range of a signal; it is presumed that very slow, large-amplitude drift in the direct current (DC) level has been removed prior to quantization without modifying the physiological content of the signal. The amplitude of individual bioelectrical waveforms ranges from $0.1 \mu\text{V}$, observed in certain types of EPs once subjected to noise reduction, to several millivolts, as observed in the ENG, ECG, and EOG.

Most bioelectrical signals recorded on the body surface have a spectral content confined to the interval well below 1 kHz, and thus the sampling rate—chosen to be at least the Nyquist rate—rarely exceeds a few kilohertz. However, since signals measured on the body surface are subjected to lowpass filtering caused by the intermediate tissue, invasively recorded signals, such as those on action potentials, generally exhibit a much higher frequency content.

In a PC-based system, signal analysis is often done locally by relying either on the internal CPU or an expansion digital signal processor (DSP) card.

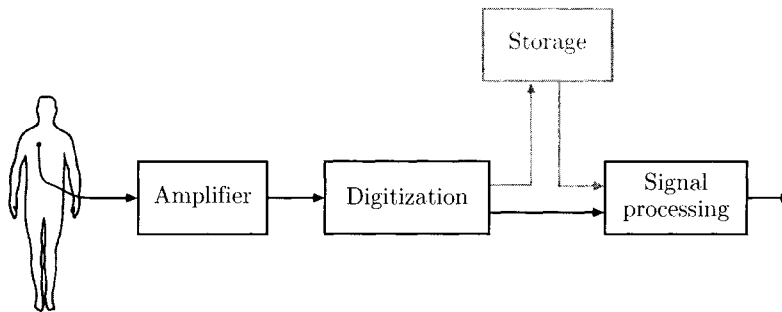


Figure 1.6: Block diagram describing the main steps in biomedical signal analysis. The signal is often processed at the time of its acquisition, but may also be stored on a local hard disk or a server on the web for later retrieval and processing.

However, with today’s availability of web-based resources, it is no longer necessary to perform the entire signal analysis locally. It is equally possible to acquire the signal at one physical location, using the PC-based system, and then to process it at another location, i.e., relying on a client/server solution [18]. Since the acquired signal in most cases is stored in a database that resides on a server, it can be advantageous to also process the signal on the server since it may offer more computational power.

1.4 Performance Evaluation

Performance evaluation is an important and challenging part of biomedical signal processing required before any algorithm can be implemented in a clinical context. Unlike many other engineering applications where the information in the signal source is known a priori, the message “sent” by a bioelectrical source is unknown and has to be unmasked in some manual way in order to render performance evaluation possible. For example, the evaluation of an algorithm for detecting heartbeats is relatively straightforward since it is an easy task for a physician to determine the times of occurrence of the heartbeats; the performance figures would then be designed to reflect how well the output of the algorithm agrees with the manually obtained times of occurrence. The performance evaluation becomes much more complicated when the goal is to develop an algorithm that computes a parameter set which accurately discriminates signals obtained from healthy subjects and patients who suffer from a particular disease. In such cases, an assessment of the output of the algorithm cannot be carried out simply because the “truth” cannot be retrieved from the observed signal. Instead, the performance may be evaluated in terms of its ability to correctly discriminate between the two